


Double Beam UV-VIS Spectrophotometer

2375

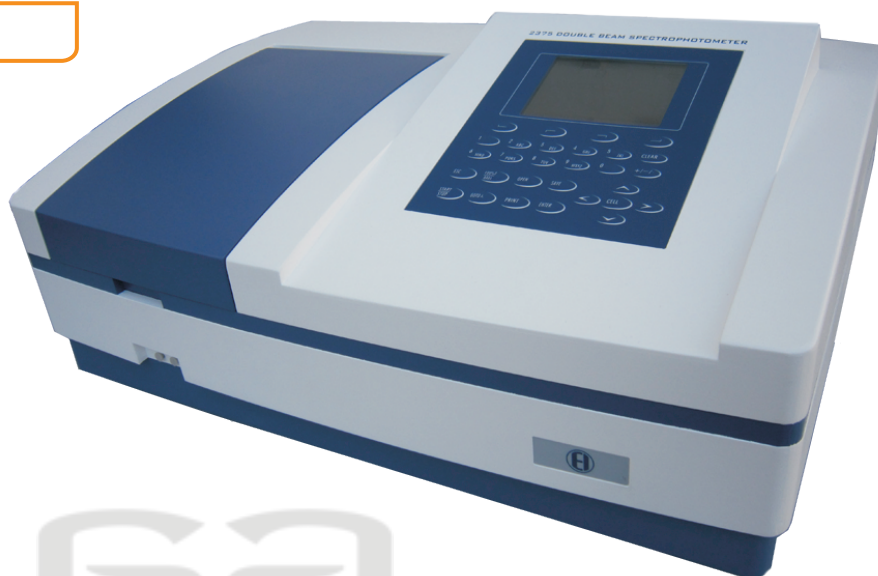

GA

1 Year
Warranty

Double Beam Spectrophotometer is a solid state microprocessor based instrument designed for quick and accurate spectrophotometric analysis of any concentration. It operates at a wavelength range of 190 nm to 1100 nm. The use of diffraction grating in the monochromator produces a linear spectrum. The grating having very high resolution of 1200 lines/mm ensures a narrow bandwidth.

The instrument is equipped with 5 Inches 320 x 240 dots graphical lcd the which makes the results easy to read. User can see the test curves on the graphical lcd screen. The system has soft touch numeric keys with complete numeric key that provides a convenient interface for entering numeric values.

The instrument output is available in terms of % Transmission (%T), Absorbance (Abs.), & Concentration (Conc.). The instrument is suitable for clinical lab applications, pharmaceutical and biochemica, as well as routing applications such as quantitative analysis, kinetics, wavelength scan, multi-wavelength and DNA/Protein analysis. The instrument has sample storage memory and printer output port for printing of data with any dot matrix printer. The PC can be connected using the USB Interface. Provision for 8 position auto cell changer with 10 mm path-length cuvette is provided.

The instrument uses the latest microprocessor technology and advanced engineering techniques so as to give enhanced accuracy and reproducibility.



- Double Beam Optics
- 320 x 240 Dots Graphical LCD
- Auto Wavelength Setting
- On-screen Standard and Kinetic Curve Display
- Tungsten/Deuterium Lamp can be turned ON/OFF Individually to Extend Lifetime
- Application Software provides complete control of the instrument from a computer through the built-in USB Port.
- Basic, WL Scan, Multi-Wavelength, Kinetic, Quantitative, DNA/Protein modes
- Pre-aligned design makes it convenient to change Lamps
- Large Sample Compartment, can accommodate 5-100 mm path-length cuvettes with optional holders. 8-Position Auto Cell Changer of 10 mm Path-length provided.



UV-VIS Spectrophotometer

Technical Data

| | |
|--------------------------|----------------------------------------------------------------------------------------------------------------------|
| MODES | Basic, Wavelength Scan, Multi Wavelength, Kinetics, Quantitative, DNA/Protein |
| WAVELENGTH RANGE | 190 - 1100 nm |
| SPECTRAL BANDWIDTH | 1.8 nm |
| OPTICAL SYSTEM | Double Beam, Grating 1200 lines/mm |
| WAVELENGTH ACCURACY | ± 0.3nm |
| WAVELENGTH REPEATABILITY | ± 0.2 nm |
| SCANNING SPEED | HI, MED, LOW, MAX 3000 nm/min |
| PHOTOMETRIC ACCURACY | ± 0.3 %T or ± 0.002A/h@1A |
| PHOTOMETRIC RANGE | 0 - 200 %T, -0.3 to 3A, 0 - 9999 Conc. |
| STRAY LIGHT | < 0.05 %T @ 220nm & 340nm |
| STABILITY | ± 0.001A/h @500 nm |
| DISPLAY | 5 Inches 320 x 240 Dots Graphical LCD |
| BASELINE FLATNESS | ± 0.001A (200 - 1000 nm) |
| SAMPLE COMPARTMENT | Standard 8 cell with automatic cell changer - 10 mm path-length. (50 mm & 100 mm path-length optional at extra cost) |
| LIGHT SOURCE | Halogen & Deuterium Lamps (Pre-Aligned) |
| OUTPUT | USB for PC Connectivity and Parallel Port for dot matrix printer |
| POWER | 230 V±10% AC, 50 Hz |
| DIMENSIONS (L x B x H) | 600 x 450 x 200 mm (Approx.) |
| WEIGHT | 22 Kg. (Approx.) |

Note: Specifications are subject to change due to continuous improvements

Product Range

Semi Auto Analyser, Double Beam UV/VIS Spectrophotometer, Single Beam UV/VIS Spectrophotometer, Flame Photometer, Haemoglobin Meter, Photo Colorimeter, pH Meter, Conductivity Meter, TDS Meter, DO Meter, Salinity Meter, Turbidity Meter, Nephelometer, Colony Counter, Karl Fischer Moisture Titrator, Fluorometer, Dissolution Test Apparatus, Disintegration Test Apparatus, Friability Apparatus, Melting Point Apparatus, Telethermometer, Temperature Indicator, Water & Soil Analysis Kit, Portable pH Meter, Portable Conductivity Meter, Portable TDS Meter, Portable DO Meter, Student Microscope, Binocular Microscope, Medical Microscope, Co-Axial Microscope.

